


LAMPIRAN 1

FLOWCHART OF EVALUATION FOR SPECIAL ACCESS APPLICATION FOR IVD MEDICAL DEVICES DURING COVID-19 EMERGENCY

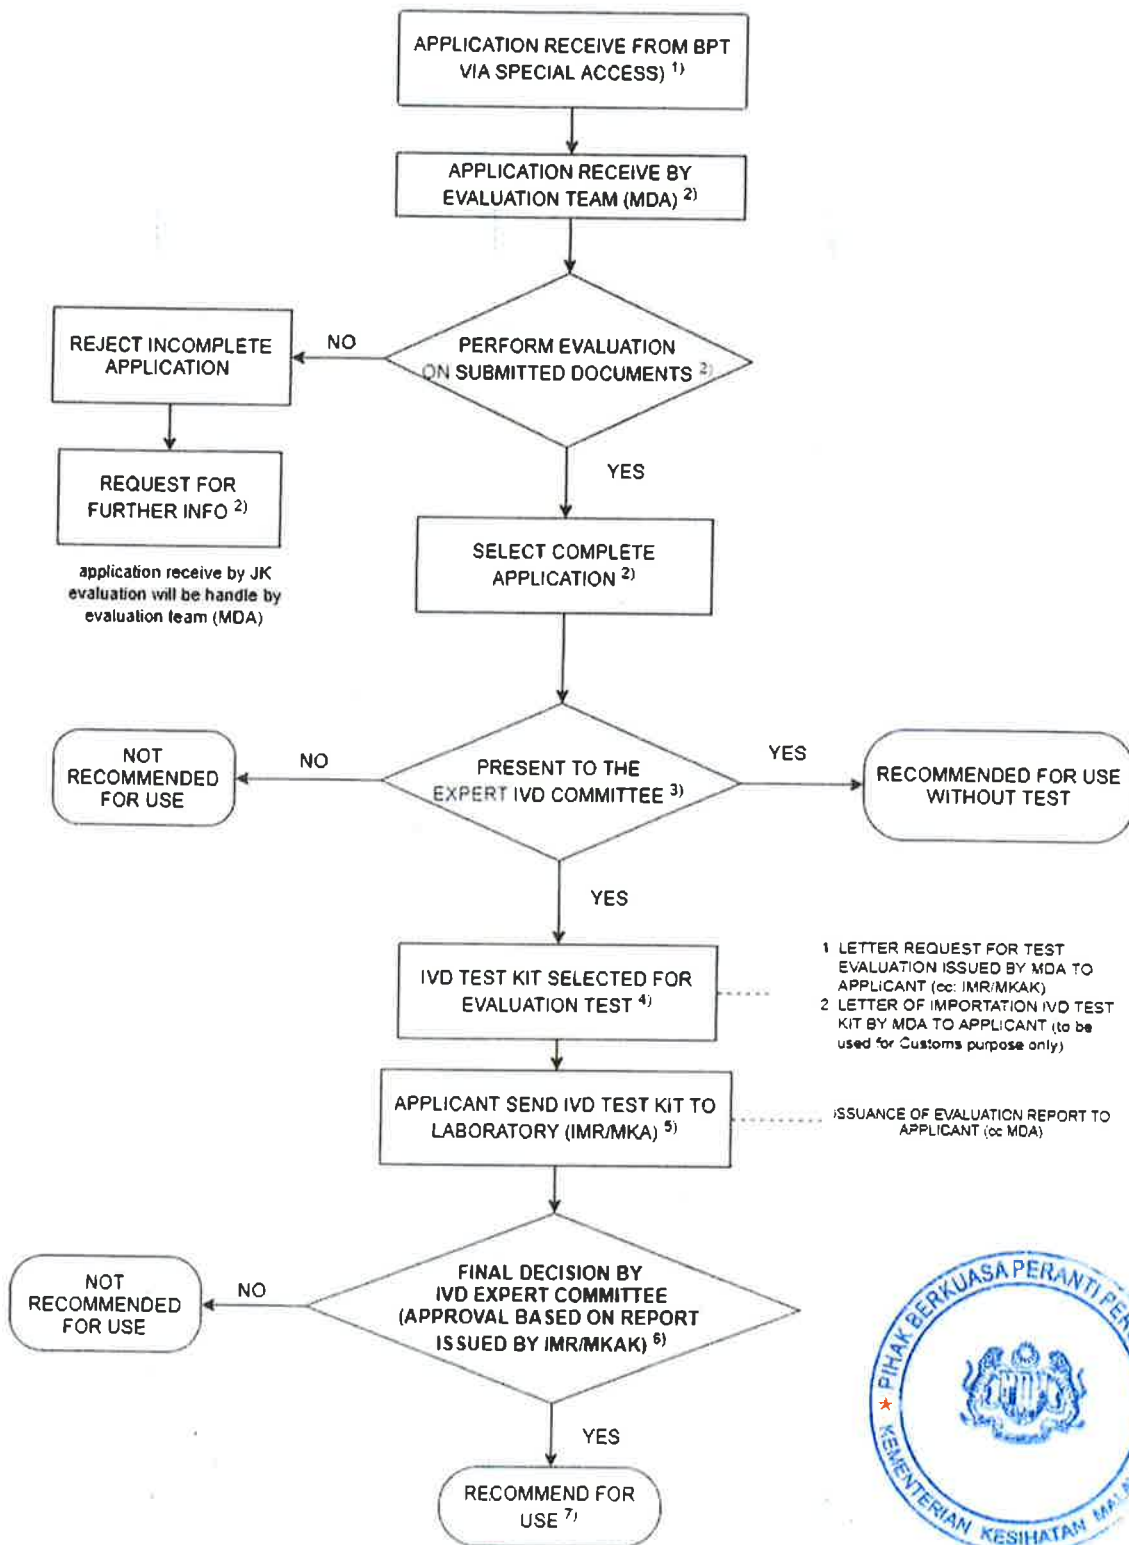

note: Inform IMR/MKAK by email kit for evaluation

AHMAD SHARIFI BIN HAMEALI
 Chief Executive
 Medical Device Authority
 Ministry Of Health Malaysia

[Handwritten signature]
 8/5/2020